


Supplementary material

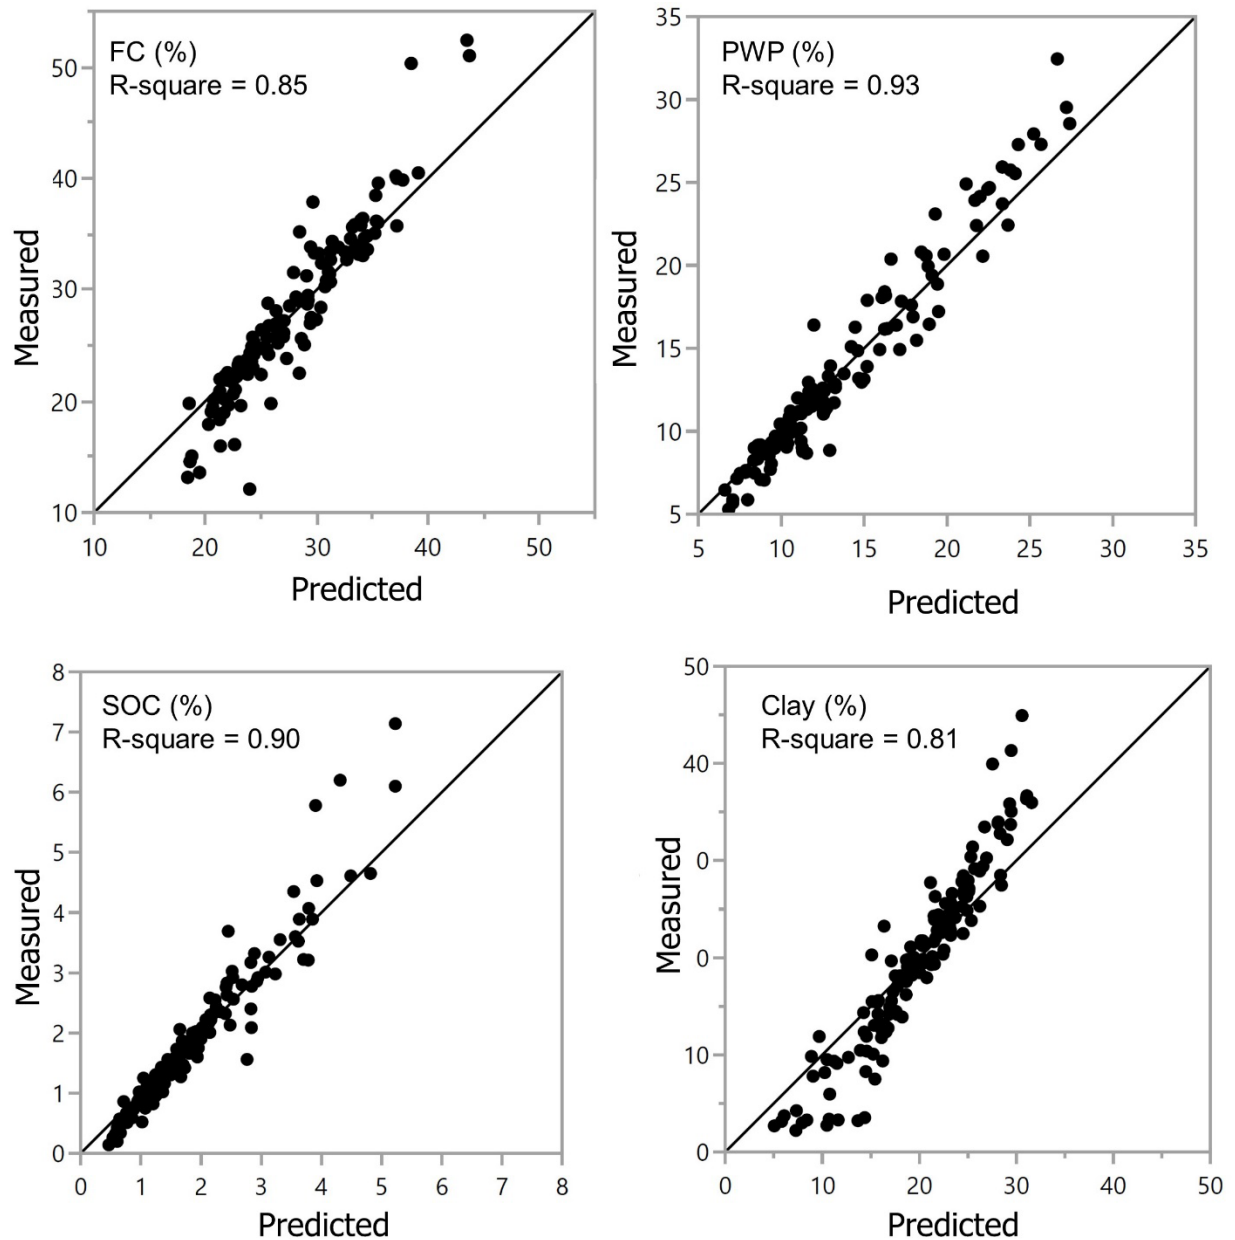

Supplementary Figure S1. Scatter plots for predicted and measured values obtained from calibrations using mid-infrared (MIR) spectroscopy coupled with random forest (RF) regression for field capacity –33 kPa (FC), permanent wilting point –1500 kPa (PWP), soil organic carbon (SOC) and clay