

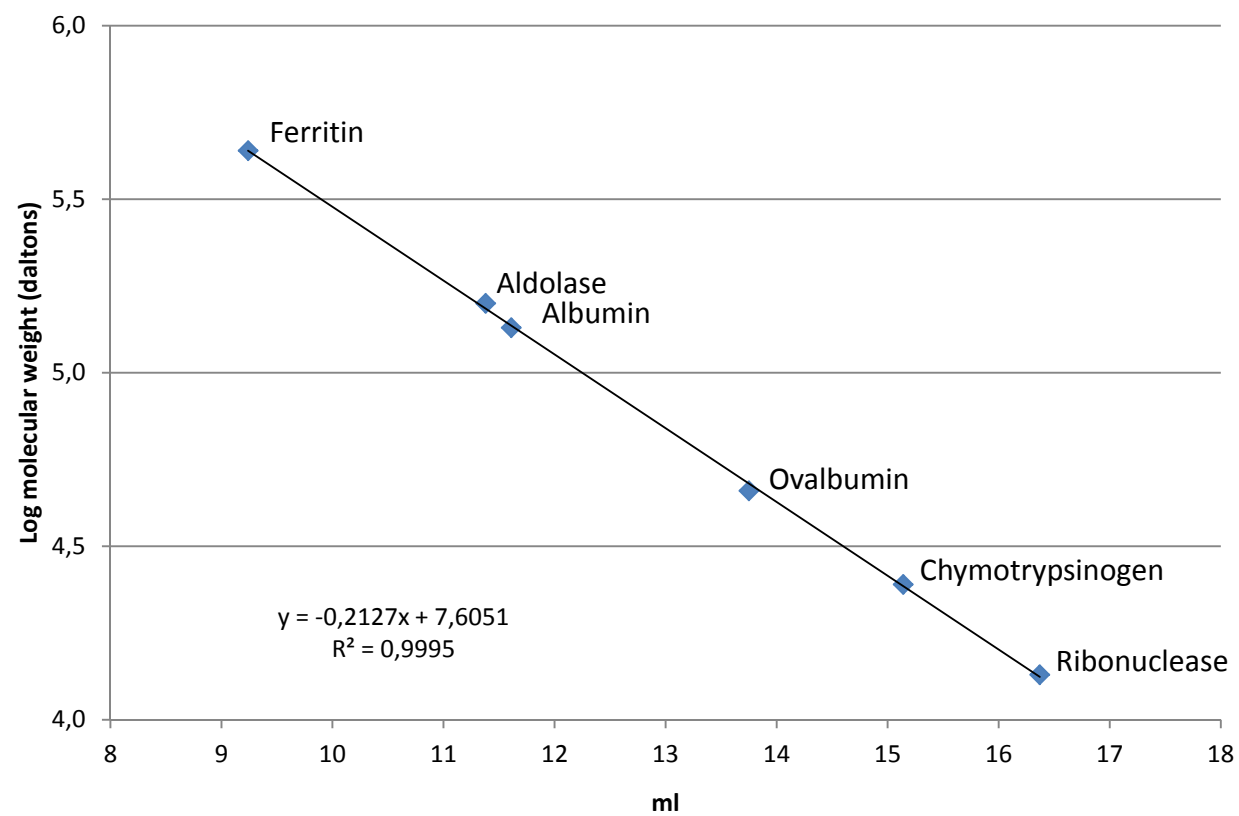


Fig. S1. Calibration curve of the Superdex-200 HR 10/30 column.